



Xenon light source



Microfluidic
Reagent Rotor



Ready-to-Use reagents.
No warm-up period
required.

7 minutes

Sample-to-answer in
3 simple steps and
approximately 7-10 minutes

18 month


18-month
shelf life

27 tests

Up to 27 tests
in a single run

Clinical Chemistry⁺

Chemistry Analyzer Celercare® V5

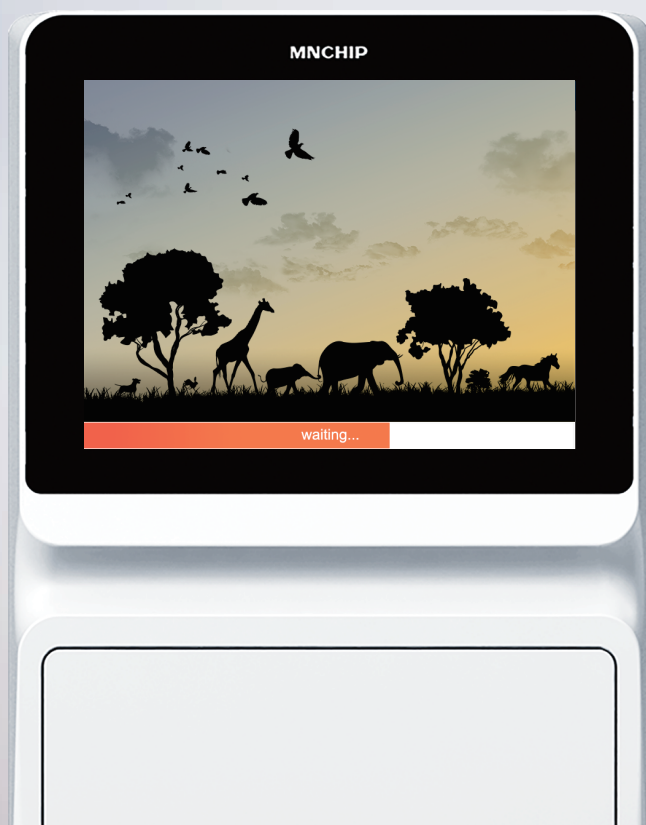

MNCHIP

21 dedicated panel options covering 44 parameters



* Calculated test value # Coming soon